

ASPTM



UP TO
27%
FASTER^{2,3} **Reduces**
COMPLIANCE ERRORS⁴

IMAGINE AN AER THAT ACCELERATES YOUR WORKFLOW⁹
AND ENHANCES COMPLIANT REPROCESSING.⁴

WELCOME TO THE FUTURE OF ENDOSCOPE REPROCESSING.

AEROFLEXTM
AUTOMATIC ENDOSCOPE
REPROCESSOR



ASP AEROFLEX™

AUTOMATIC ENDOSCOPE REPROCESSOR

Accelerates WORKFLOW⁹ and Enhances COMPLIANCE⁴

FASTEST CYCLE TIME⁵

- At 22 minutes, ASP AEROFLEX™ AER offers the fastest complete cycle time of any AER currently sold⁵
- Up To 27% Faster Cycle than Olympus OER-Pro™ 2,3 and up to 15% Faster than Medivators DSD EDGE™1,3
- Save up to 280 hours per year of valuable staff time⁶
- Automation of critical steps streamlines workflow, allowing you to turn your scope inventory faster and perform more procedures.

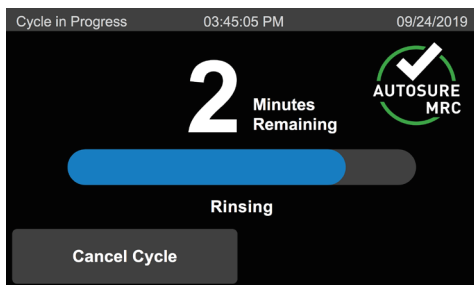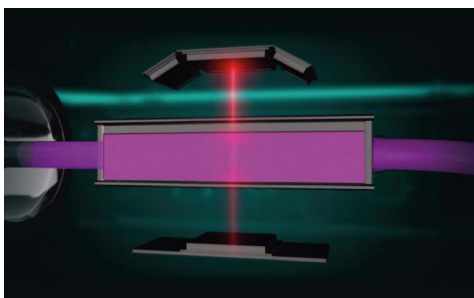

EXCLUSIVE AUTOSURE™ MRC⁷ MONITOR

- Built into the ASP AEROFLEX™ AER, eliminating manual test strips
- Reduce the opportunity for human errors related to manual test strip use
- Reduces patient risk associated with test strip errors¹¹
- MRC testing can't be skipped
- Ensures biocide is above MRC every cycle
- Cycle won't start if biocide doesn't meet MRC
- Always uses validated chemistry
- Reduces staff exposure to chemicals

EXCLUSIVE DUODENOSCOPE AUTO-DETECTION FEATURE

- Extra precaution for high-risk scopes¹⁰
- Automatically detects duodenoscopes and runs a special cycle to ensure proper high-level disinfection¹⁰



AEROFLEX™

AUTOMATIC ENDOSCOPE REPROCESSOR



ASP AEROZYME XTRA™
MULTI ENZYMATIC DETERGENT



ASP AERO-OPA™
ORTHO-PHTHALALDEHYDE
SOLUTION



AUTOSURE™
MRC REAGENT



Automated, Audit Ready Records

- MRC STATUS AUTOMATICALLY DOCUMENTED EVERY CYCLE
- EVERY CYCLE MONITORED AUTOMATICALLY
- AUTOMATICALLY PRINTS REPORT AT COMPLETION OF EACH CYCLE
- HANG TIME ALERTS, CYCLE HISTORY AND SCOPE USAGE REPORTS AVAILABLE THROUGH ASP ACCESS™ TECHNOLOGY



AEROFLEX™

AUTOMATIC ENDOSCOPE REPROCESSOR



Important information: Prior to use, refer to the complete instructions for use supplied with the device(s) for proper use, indications, contraindications, warnings and precautions.

asp.com

ASP Advanced
Sterilization
Products

ASP International GmbH, Zug Branch
Bahnhofstrasse 2, Zug 6300, Switzerland
©ASP 2021. All Rights Reserved.



ASP International GmbH, Zweigniederlassung Zug
Gubelstrasse 34, 6300 Zug, Switzerland

**Protecting patients during
their most critical moments**

¹ The ASP AEROFLEX™ AER 22 minute cycle saves 3 minutes compared to the Medivators DSD Edge 25 minute cycle time and saves up to a minute in test strip time (refer to footnote 3) for a total time savings of up to 4 minutes. ² The ASP AEROFLEX™ AER 22 minute cycle saves 7 minutes compared to the Olympus OER Pro 29 minute cycle when used with ALDAHOL 1.8 high-level disinfectant and 1 minute in test strip time (refer to footnote 3) for a total time savings of 8 minutes. ³ Test strip savings time calculated from C.L. Ofstead et al. / American Journal of Infection Control, Accessed 12/12/2019 [www.ajicjournal.org/article/S0196-6553\(19\)30849-1/fulltext](http://www.ajicjournal.org/article/S0196-6553(19)30849-1/fulltext) (2019) 1–7, Table 2. ⁴ ASP AEROFLEX™ AER with AUTOSURE™ MRC Monitor may enhance compliance to ASP AERO-OPA™ and ASP AEROFLEX™ AER instructions for use (IFU), professional society guidelines for endoscope reprocessing, healthcare facility policies and procedures for endoscope reprocessing and government and local environmental regulations for chemical disposal. ASP AEROFLEX™ AER with AUTOSURE™ MRC Monitor may enhance compliance through automated features for HLD minimum recommended concentration (MRC) testing, verified chemistry confirmation, endoscope reprocessing record keeping and neutralization of ASP AERO-OPA™ before disposal. ⁵ In countries where distributed. Includes wash, high-level disinfection, rinses, MRC testing and alcohol flush. For all qualified endoscopes except duodenoscopes which require additional time. Assuming nominal conditions for water pressure, flow rate and temperature. ⁶ Assumes savings of 8 minutes per cycle, 9 non-duodenoscope cycles per day, 250 days per year (when compared to the Olympus OER Pro; 29 minute cycle when used with ALDAHOL 1.8 high-level disinfectant (7 minute cycle time savings plus 1 minute test strip time savings.)) ⁷ Minimum Recommended Concentration (MRC). Measurement of the Minimum Recommended Concentration level of active ingredient in the biocide. ⁸ Assumes \$.90 per test strip, 9 non-duodenoscope cycles per day, 250 days per year. ⁹ Workflow refers to the testing of chemistry, it does not refer to pre-cleaning/manual cleaning. ¹⁰ Extended Duodenoscope cycle is 36 minutes. ¹¹ C.L. Ofstead et al. / American Journal of Infection Control (2019) 1–7, Accessed 12/12/2019 [www.ajicjournal.org/article/S0196-6553\(19\)30849-1/fulltext](http://www.ajicjournal.org/article/S0196-6553(19)30849-1/fulltext)